

Whole blood processing kit

P01 - Sample stabilisation



Preparation phase:

Aliquot cryogenic vials¹ with **Cytodelics Stabiliser equal the planned blood sample volume. Store at 5–8°C until sampling (up to 2 years). Identify dispensed volume on the label.**

Protocol:

1. Bring tubes pre-filled with the Stabiliser **to room temperature** (5 – 10 minutes).
2. Transfer equal **blood** volume to the cryogenic vial (RATIO 1:1).
3. **Mix** the blood sample with the Stabiliser **by flipping** the vial 10-15 times. **Do not** vortex!
4. Incubate at room temperature for 10 minutes.
5. Store the sample until further processing at:
 - a. $\leq -80^{\circ}\text{C}$ (up to 1 year);
 - b. $\leq -20^{\circ}\text{C}$ (up to 2 months), then transfer to the ultra-low freezer ($\leq -80^{\circ}\text{C}$) as soon as possible and keep there until further processing (up to 1 year);
 - c. or place on **dry ice** and transfer to to the ultra-low freezer ($\leq -80^{\circ}\text{C}$) as soon as possible and keep there until further processing (up to 1 year).

¹ Choose cryogenic vial with nominal volume of approx. 3-times of the planned blood sample.

Whole blood processing kit

P01 - Processing after sample thawing

1. **Calculate** the required volume of the **Fixation Buffer** (total volume of blood processed within one batch multiplied by factor 10) and **prepare** it by mixing equal volumes of
 - a. Fix-concentrate
 - b. Fix-Diluent
2. **Dispense** the **Fixation Buffer** (10-times volume of preserved blood; do not count on the Stabiliser volume²) to tubes and let to equilibrate to room temperature (approx. 5 minutes).
3. **Thaw** blood samples preserved in the Stabiliser by quickly heating on water bath or heat block set to 37°C (approx. 1 minute).
4. **Transfer** {blood+Stabiliser} mixture to the tube with the Fixation buffer, set the timer, and **incubate** for **15 minutes** at **room temperature**. Vortex multiple times throughout.
5. **Add** 1-time concentrated **LYSIS buffer** (40-times volume of the blood sample³), **mix** well by inverting tube multiple times, and **incubate** at room temperature for minimum of **15 to 20 minutes** until a complete erythrocytes' lysis.
6. **Centrifuge** at **300g for 5 to 10 minutes**⁴.
7. **Aspirate the supernatant**, according to the size of the sample, down to:
 - approx. mark 5.0-7.5 ml in 50mL tube, and before the next step, proceed as follows:
 - i. transfer to a 15mL tube,
 - ii. rinse twice with 2.0 ml of the **LYSIS buffer** and transfer to the 15mL tube,
 - iii. centrifuge at 300g for 5 minutes,
 - iv. aspirate the remaining volume down to approx. mark 0.5 ml.



² E.g., for 1.0 ml of blood preserved in 1.0 ml of Stabiliser use **10.0 ml of the Fixation Buffer**, i.e., 10-times volume of the blood.

³ E.g., for 1.0 ml of blood and 10.0 ml of Fixation Buffer use **40.0 ml of the LYSIS buffer**.

⁴ Set the centrifugation timing according to the liquid column height in the tube and rotor size. The timing should increase with shorter rotor diameter and/or more liquid (higher liquid column) per tube.

Whole blood processing kit

- approx. mark 0.5 ml in a 15mL tube (for samples with original volume up to 250µl blood processed in the 15mL tube from the beginning),
 - “ring” on the 5mL “FACS” tube, leaving a minimum of 100 µl of supernatant over the pellet.
8. Break the pellet by vortexing and **add** 1-time concentrated **WASH buffer** (40-times the volume of the blood sample⁵).
 9. **Centrifuge at 300g for 5 to 10 minutes**⁶.
 10. **Gently aspirate** the supernatant down to:
 - a. approx. mark 0.25 ml (15mL tube)
 - b. ring” on the 5mL “FACS” tube leaving approx. 100 µl of supernatant over the pellet.

Do not decant!

11. Proceed with:
 - a. sample staining and acquisition,
 - b. **cryogenic preservation** in CRYO#20 buffer at $\leq -80^{\circ}\text{C}$.

For thawing, proceed as follows:

- i. Thaw the sample in a range from 20°C to 37°C (ideally on a heat block),
- ii. Process according to your downstream application⁷.



⁵ E.g., for 1.0 ml of blood, 10.0 ml of Fixation Buffer, and 40ml of LYSIS buffer use **40.0 ml of the WASH buffer**.

⁶ Set the centrifugation timing according to the liquid column height in the tube and rotor size. The timing should increase with shorter rotor diameter and/or more liquid (higher liquid column) per tube.

⁷ You may stain without the washing step and acquire; however, we recommend to test compatibility of your staining panel. Before the staining, centrifugate the sample at 300-400g/ \approx 5 min and remove some of the supernatant to optimize volume of the Ab-cocktail and antibodies consumption.

Whole blood processing kit

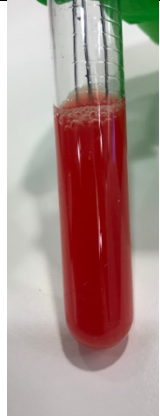





Scaling ratios		
Blood	1 : 1	Cytodelics Stabiliser
Blood	1 : 10	Fixation buffer
Blood	1 : 40	LYSIS buffer
Blood	1 : 40	WASH buffer
Blood	1 : 0.5 - 1	CRYO#20

Examples of recommended processing conditions						
Blood sample volume	Fix buffer volume	LYSIS buffer volume	WASH buffer volume	Recommended processing tube size		CRYO#20 volume
				First wash	All consequent washes	
100 µl	1.0 ml	4.0 ml	4.0 ml	10 – 15 ml	5-15 ml	100 µl
250 µl	2.5 ml	10 ml	10 ml	15 ml	15 ml	100 µl
500 µl	5.0 ml	20.0 ml	20.0 ml †	50 ml *	15 ml	250 µl
1.0 ml	10.0 ml	39.0 ml	40.0 ml †	50 ml *	15 ml	500 µl

* To achieve optimal cell yields execute only first spin after Fix&Lyse step in 50 ml tube, aspirate to mark 5 ml or above (not below 5 ml mark), transfer to 15 ml tube and continue with altered WASH buffer volumes.

† In case you decide to run all consequent processing steps in 15 ml tube, use 14 ml of WASH buffer and adjust number of washing steps based on pellet color. Typically, only one more washing step is required.

Guide on decision of RBCs lysis step duration:

Time after addition of LYSIS buffer						
	0 min	5-6 min	10 min	15 min	20 min	35 min
	No	No	No	OK	OK	OK

Conditions: Fresh whole blood fixed for 15 min at RT followed by addition of LYSIS buffer for indicated time